



Fluorescence

Table of Contents


Table of Contents	1
Overview	2
Chip Design	3
Milling Guidelines	4
Milling Guidelines	4
Notes	4
Milling Instructions	5
Flow Layer	5
Control Layer	5
Testing Protocol	6
Flow Layer Setup	6
Control Layer Setup	7
Testing the Chip	7
Setup	7
Running the chip	7
Cleaning the Chip	8

Overview

Fluorescence

Designed by Dinithi Samarasekera



Date Completed: 10/25/2017

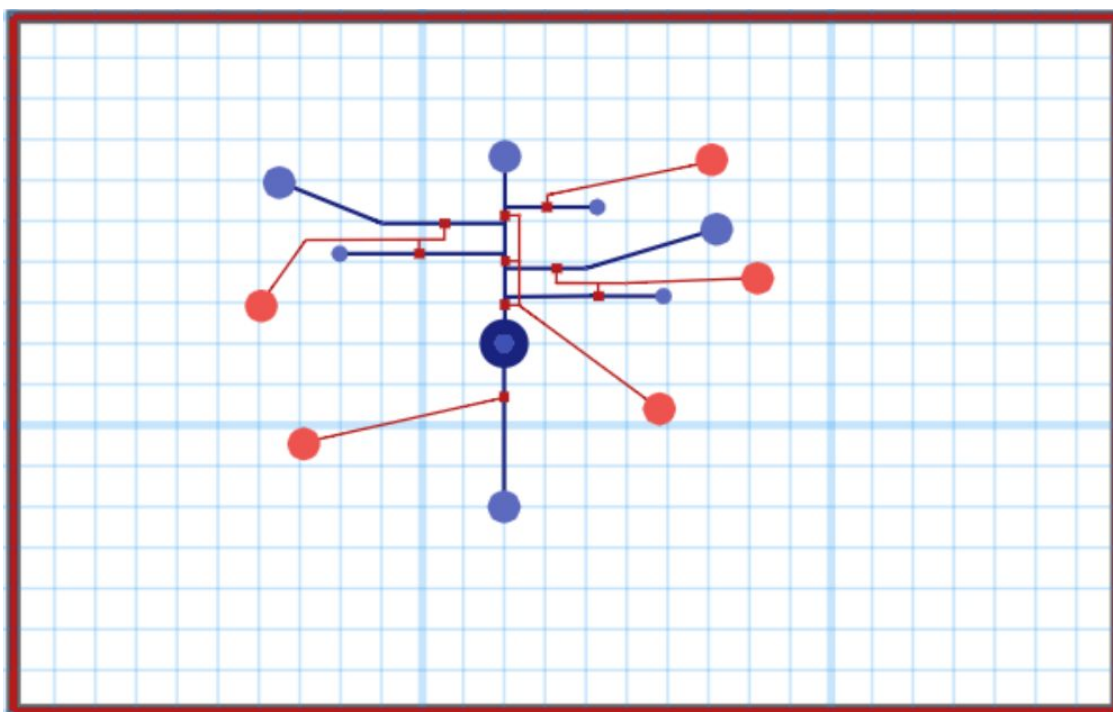


Fluorescence is commonly used as a quantifiable marker in synthetic biology procedures. Following the completion of a protocol, for example an assay test, samples are tested in a plate reader and the results analysed.

This microfluidic chip is designed to perform a Cell-free Toehold test, however it can be adapted to perform alternative fluorescent tests as desired. The metering primitive dispenses accurate ratio volumes of various substances. These are pushed into the central well which matches the dimensions of a 96-well plate. The chip can then be read in a plate reader with the use of an adapted skirt.

Chip Design

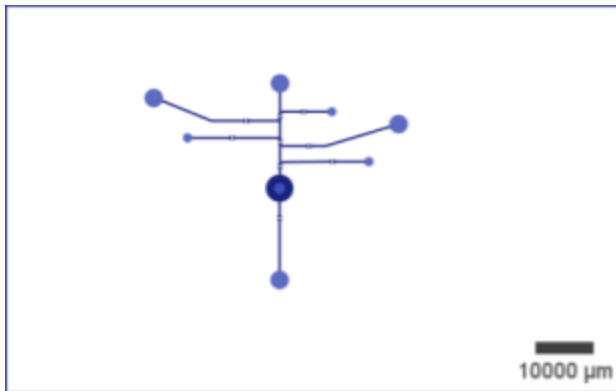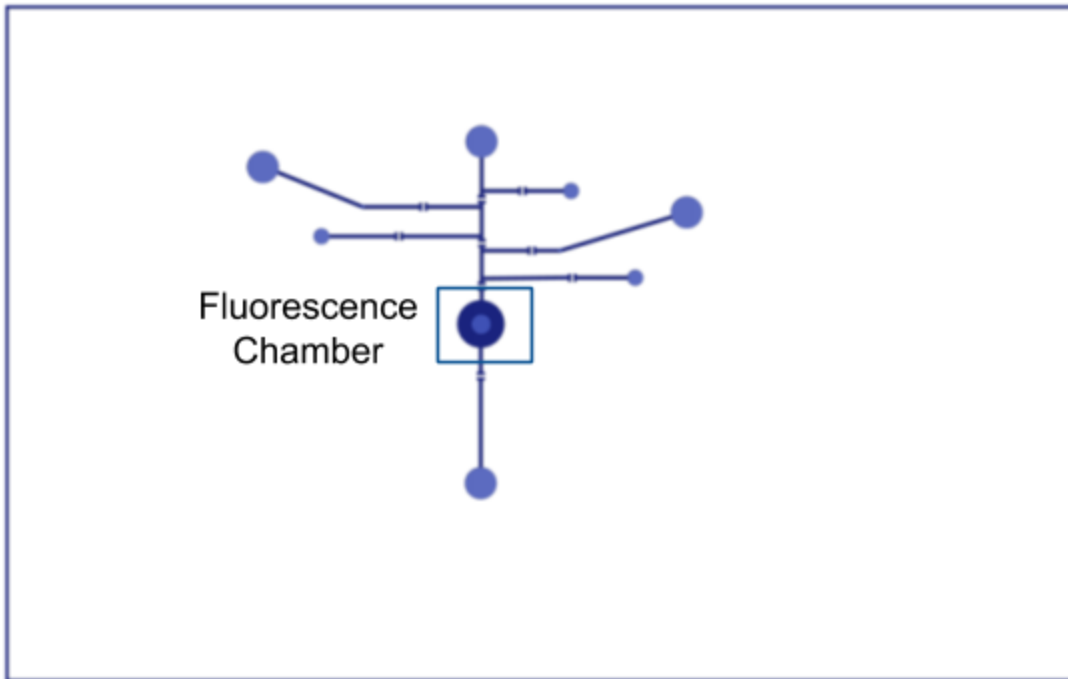


Flow Layer

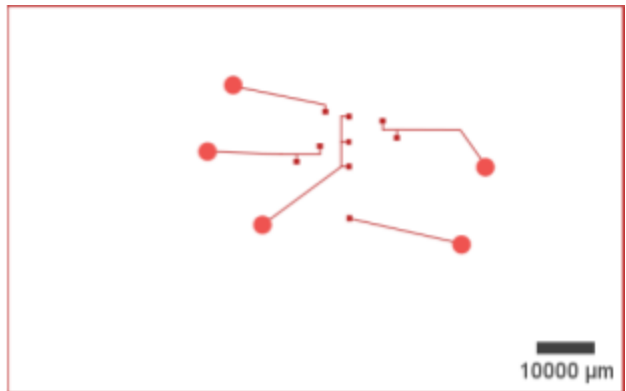


Control Layer

Milling Guidelines

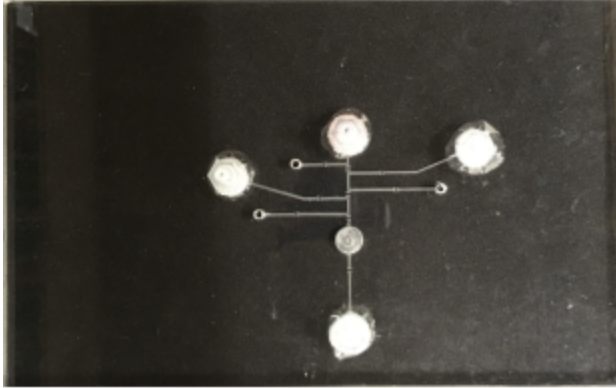

Flow Layer

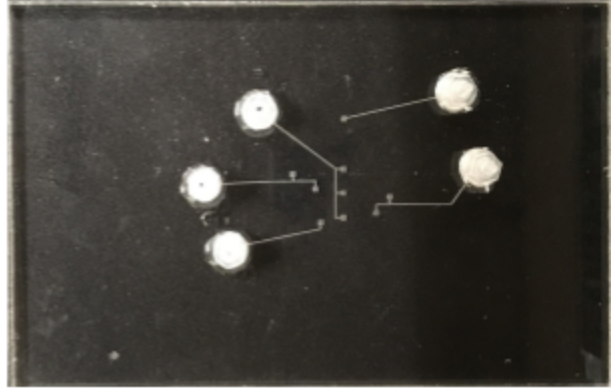

Control Layer


Milling Guidelines

For a comprehensive guide to milling click [here](#). For a list of tool parameters click [here](#).

Notes

1. This chip should be milled on medium or thick polycarbonate ($2.75\text{mm} < Z_{\text{Polycarbonate}}$).
2. This chip requires thick PDMS ($1.0\text{mm} < Z_{\text{PDMS}} < 1.5\text{mm}$)

All the required SVGs for milling this chip are provided in the ZIP file. The layer, depth, and tool required for each SVG is listed in the file name. Below is a key describing how to read an SVG file name:

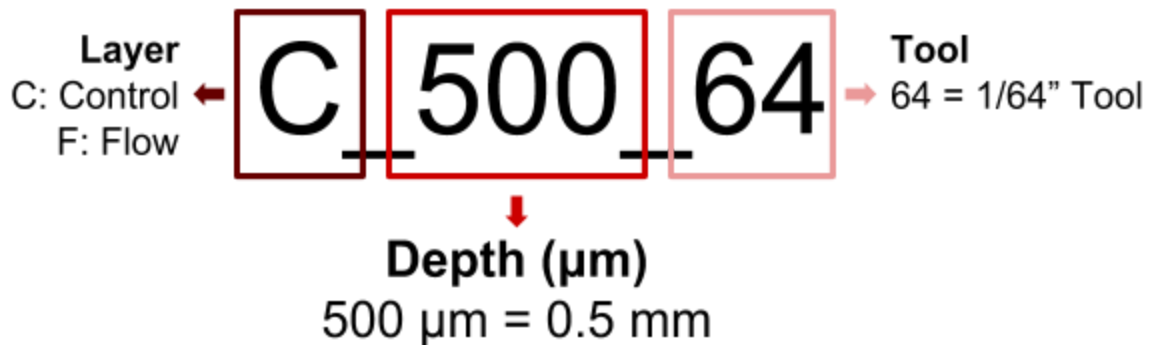

Milling Instructions


Mill the layers in the order they are listed with the correct depths and using the correct tools.

Flow Layer	
Order	Layer Name
1.	F_CHAMBER_16
2.	F_500_64
3.	F_PORTS_8
4.	Border

Control Layer	
Order	Layer Name
1.	C_300_100
2.	C_PORTS_8
3.	Border

Testing Protocol


Flow Layer Setup

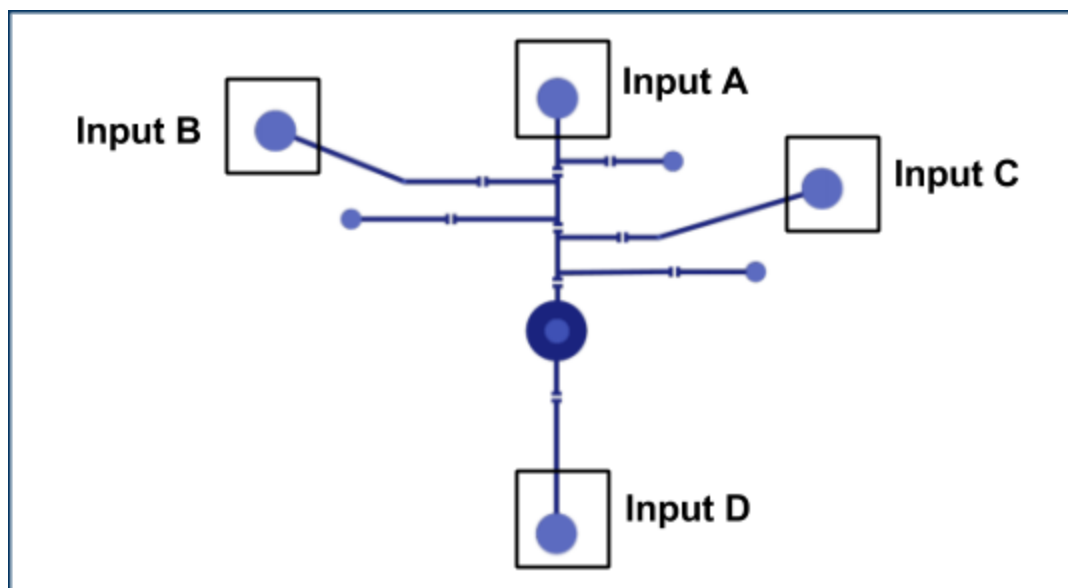

Inputs		
Name	Liquid	Flow Rate
A	Oil	0.2 mL/hour
B	Toehold	0.2mL/hour
C	Trigger RNA	0.2mL/hour
D	Master Mix	0.3mL/hour

Outputs	
Name	Liquid
a	Fluorescent Solution

Control Layer Setup

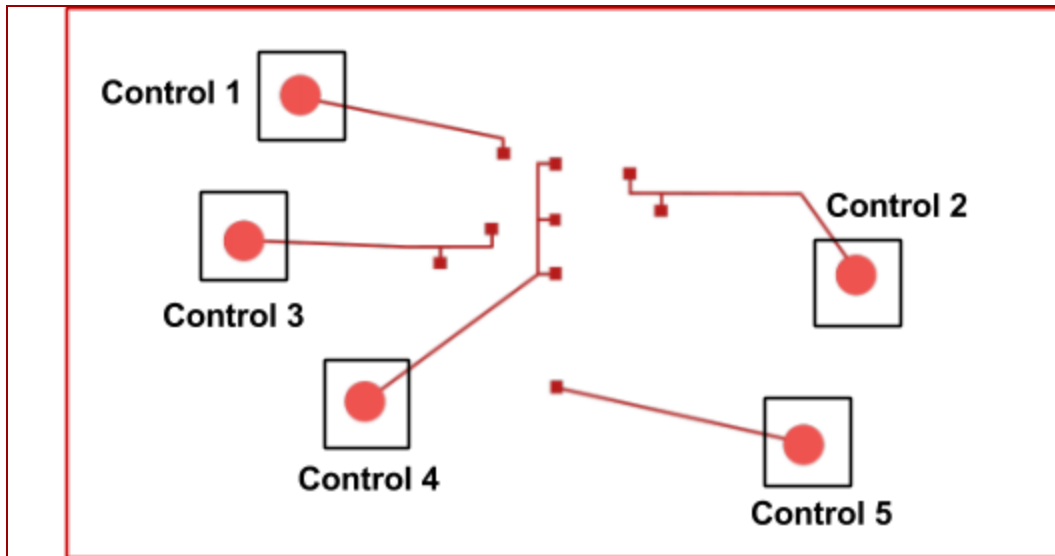

Testing the Chip

Setup

1. Prepare 4 syringes
 - a. 3 filled with colored water
 - b. 1 filled with mineral oil
 - c. 5 empty control syringes
2. Attach the syringes containing coloured water to inputs B,C and D
3. Attach the syringe containing oil to input A
4. Attach the control syringes to all five control layer outputs

Running the chip

5. Open Controls 1 ,2 and 3; you should feel significant resistance while you open these control valves
6. Begin flowing Inputs A, B, and C
7. When the metered segment for each input is filled, stop the fluid flow and close their corresponding Control line
8. Open Control 4 and begin flowing Input A
9. When the oil is close to the final valve before entering the chamber, stop flowing Input A and close Control 4
10. Open Control 5 and flow Input D until the chamber is filled to a satisfactory level
11. Halt the flow of Input D and then close Control 5

Cleaning the Chip

12. Disconnect all syringes carefully
13. Clean the chip following the oil & water protocol listed [here](#)
14. Store your chip as detailed in the cleaning protocol